



Transporting All Samples and Controls to the Research Flow Cytometry Facility (RFCF) for Analysis and Sorting BSL1, BSL2, BSL2+

1. Sealed Cap Tube: ALL samples must be placed in sealed capped tubes.

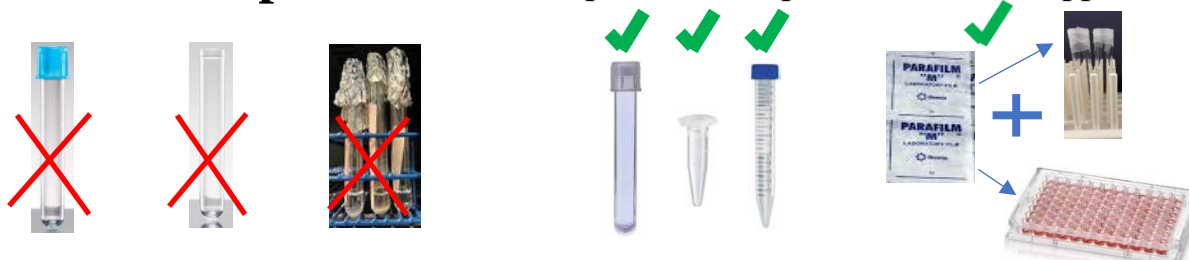

2. Secondary Leak Proof Container: The sealed capped tube must be placed into a secondary leak-proof container with absorbent between containers.

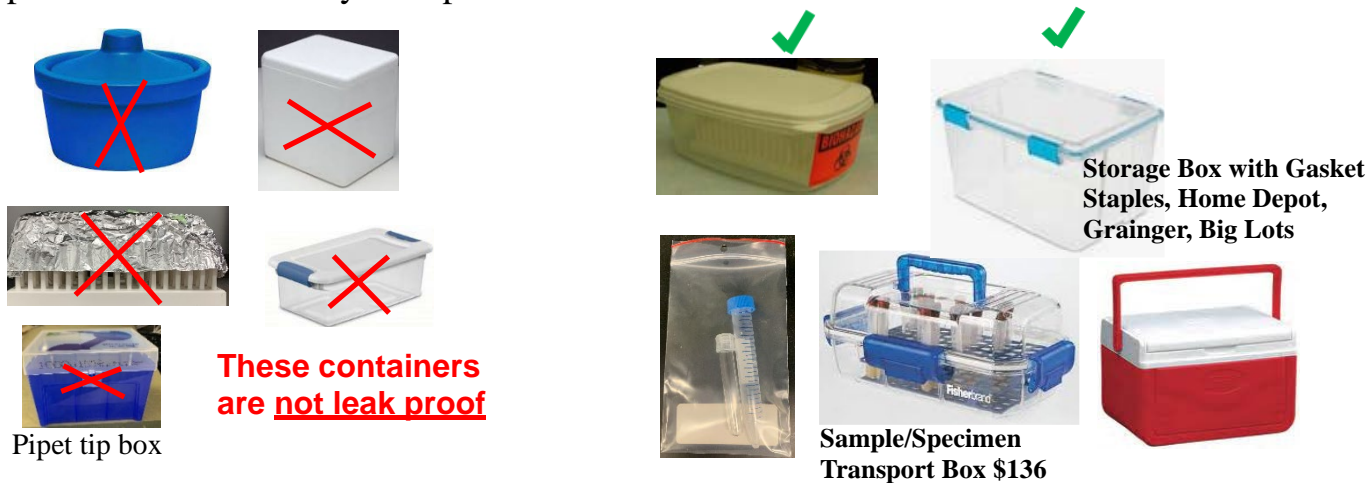


3. Biohazard Sticker: If the sample is a Biohazard (BSL2, BSL2+), it must be labeled with the biohazard symbol.



Examples

Sealed Leak Proof secondary container can be placed in ice.

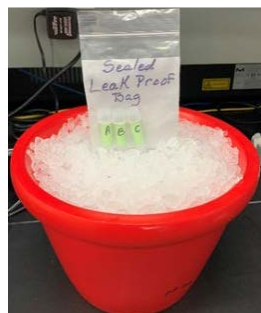

Sealed samples can be placed in a container with ice which is then placed in sealed LEAK PROOF secondary container with absorbent.

